

This Page Is Inserted by IFW Operations  
and is not a part of the Official Record

## BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

IMAGES ARE BEST AVAILABLE COPY.

As rescanning documents *will not* correct images,  
please do not report the images to the  
Image Problem Mailbox.

See for example, Seng and Dr. Z.  
System of Staped  
Therapy

each position  
adjustable

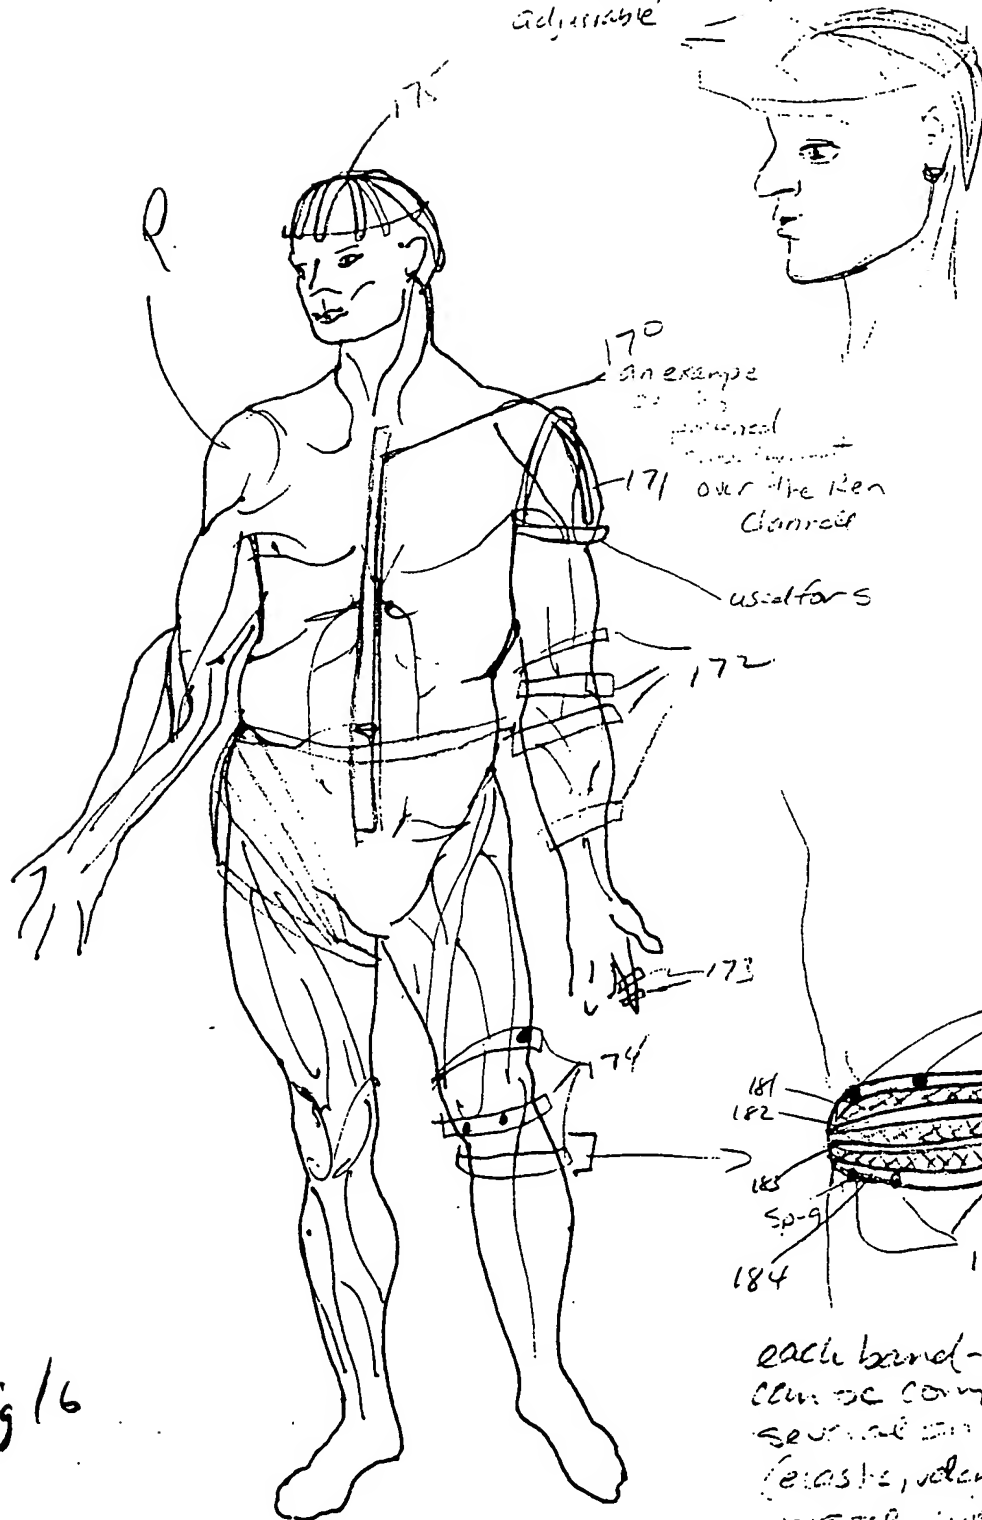


Fig 16

each band - all adjustable  
element composed of  
several smaller straps  
(elastic, velcro, pliable shear  
metal, with adjustable  
position of magnets, polariz  
panels, moxa and/or  
medicaments utilizing the  
techniques + principles of the previously described applicat.

10449393-112609

For  
Hip  
knee,  
shoulder  
injury or  
replacement  
therapy

These straps can be  
arranged in many  
different configurations  
and designs for each  
individual's needs and  
anatomy, and can be  
used in conjunction  
with other therapy devices  
if desired.

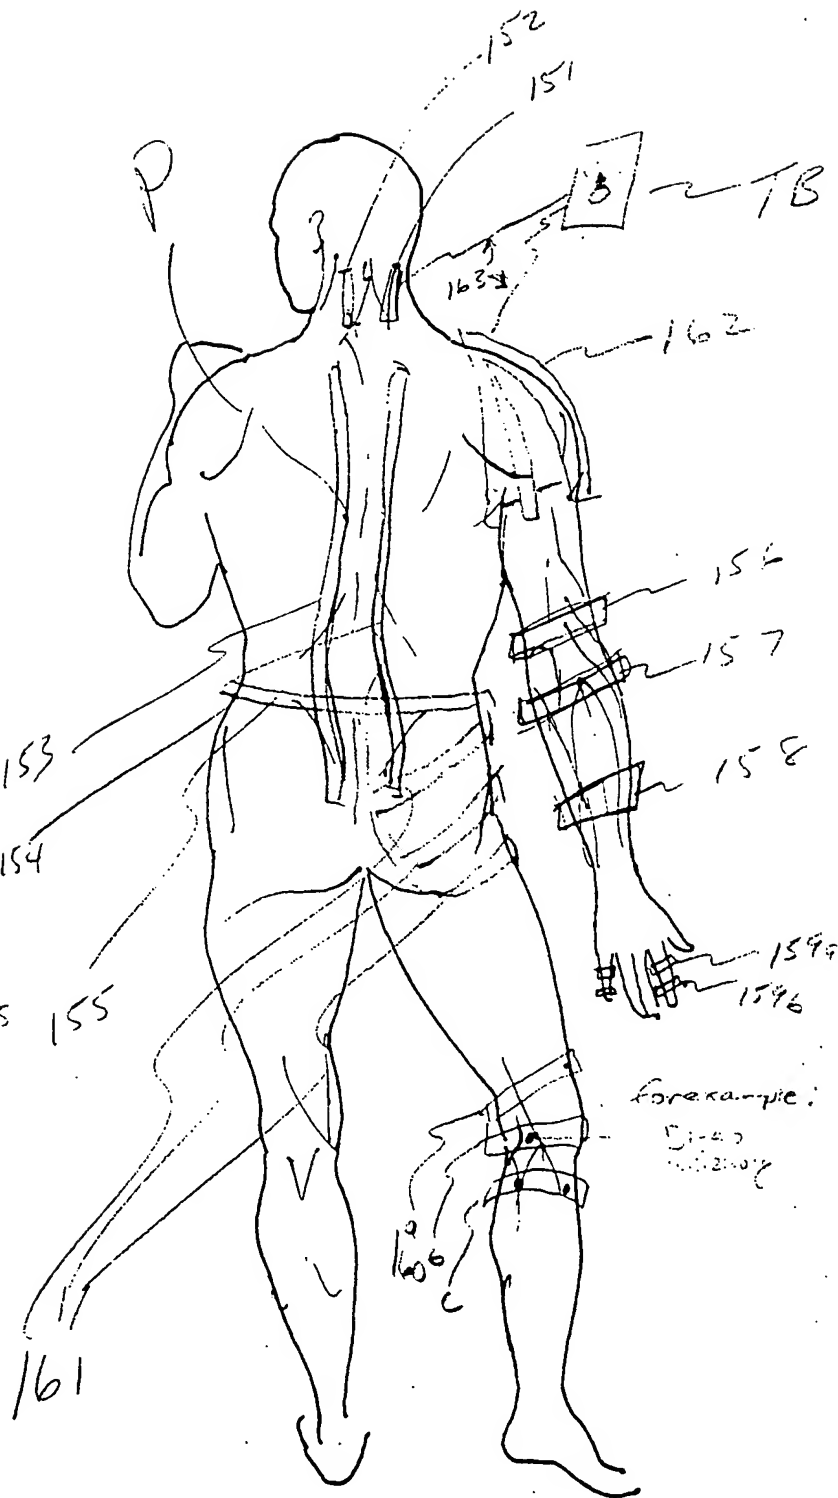


Fig. 15



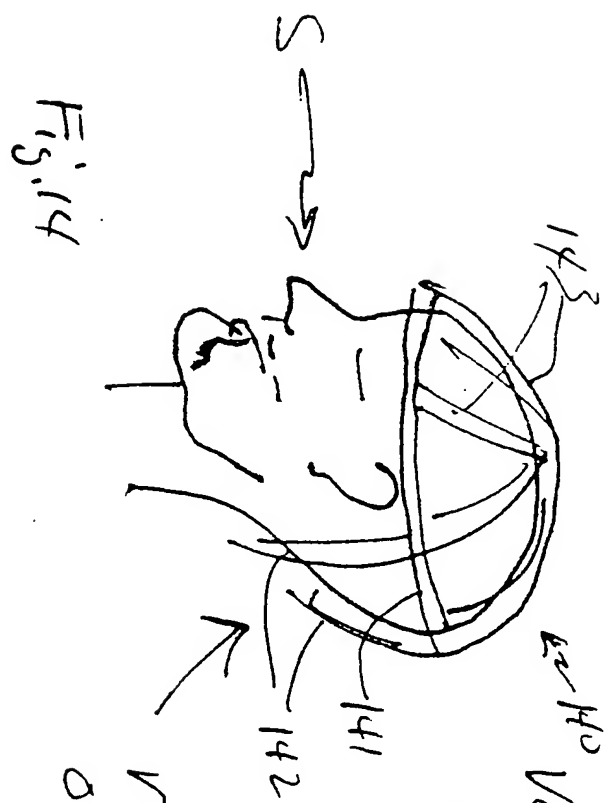


Fig. 14

143  
141  
142  
144  
S  
Velar  
+ totally adjustable  
+ interchangeable to make  
remind you of something out  
of the Baker museum?

09449393 113699

PRINT OF DRAWINGS  
AS ORIGINALLY FILED

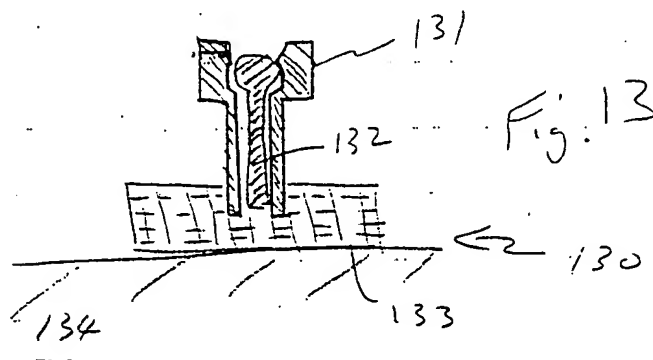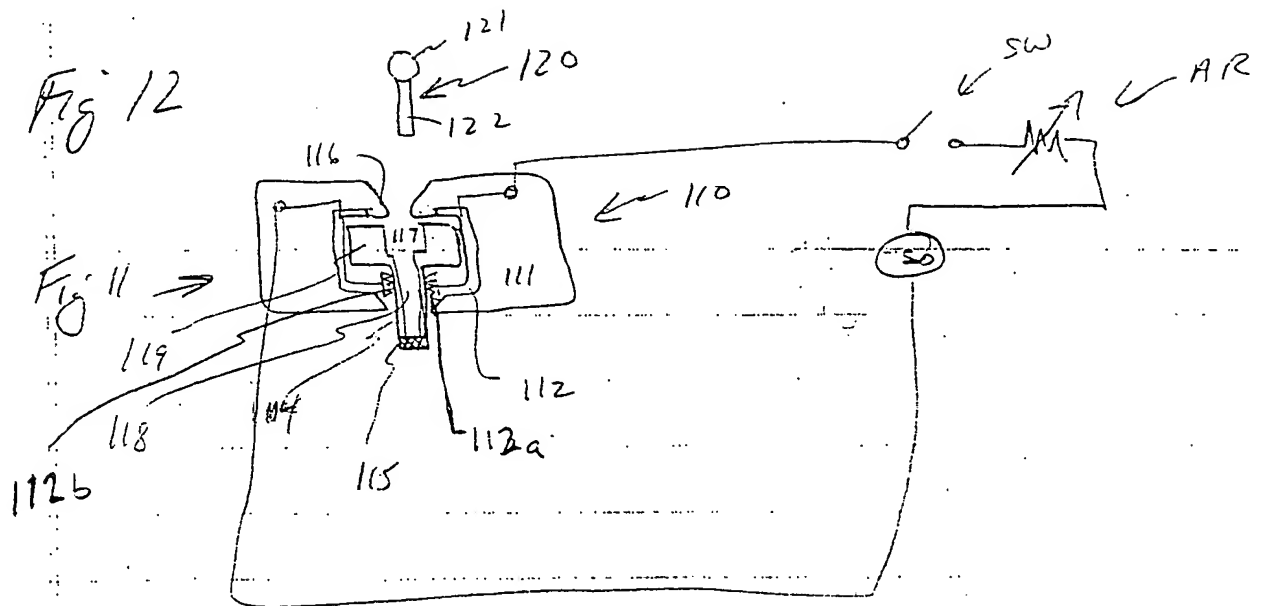

0449393-12509

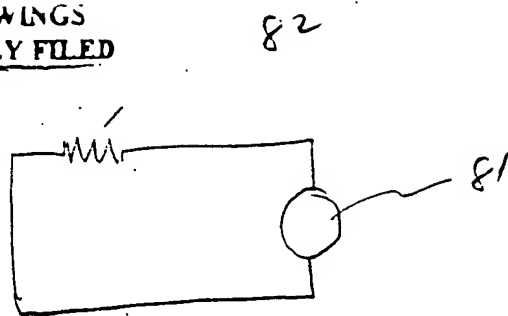


Fig. 7

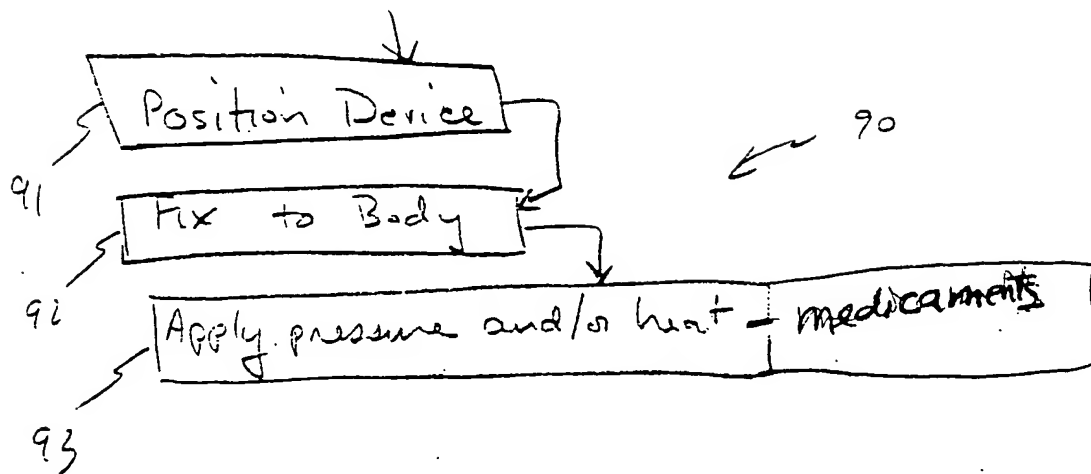


Fig. 8

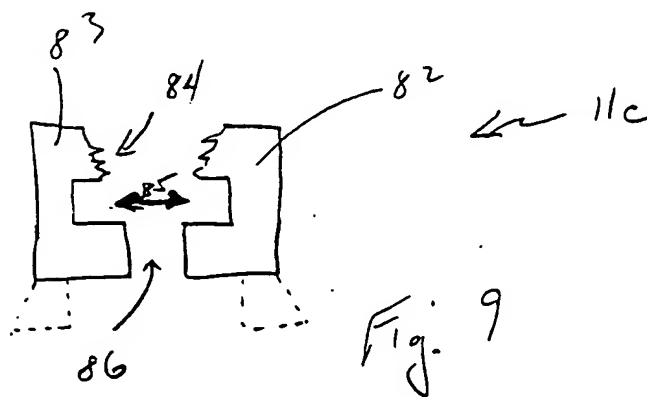


Fig. 9

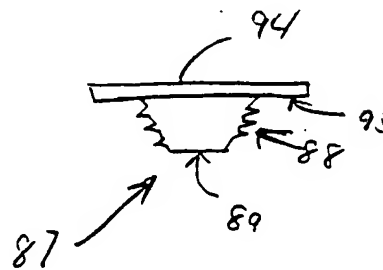


Fig. 10

00449393-112699

PRINT OF DRAWINGS  
AS ORIGINALLY FILED

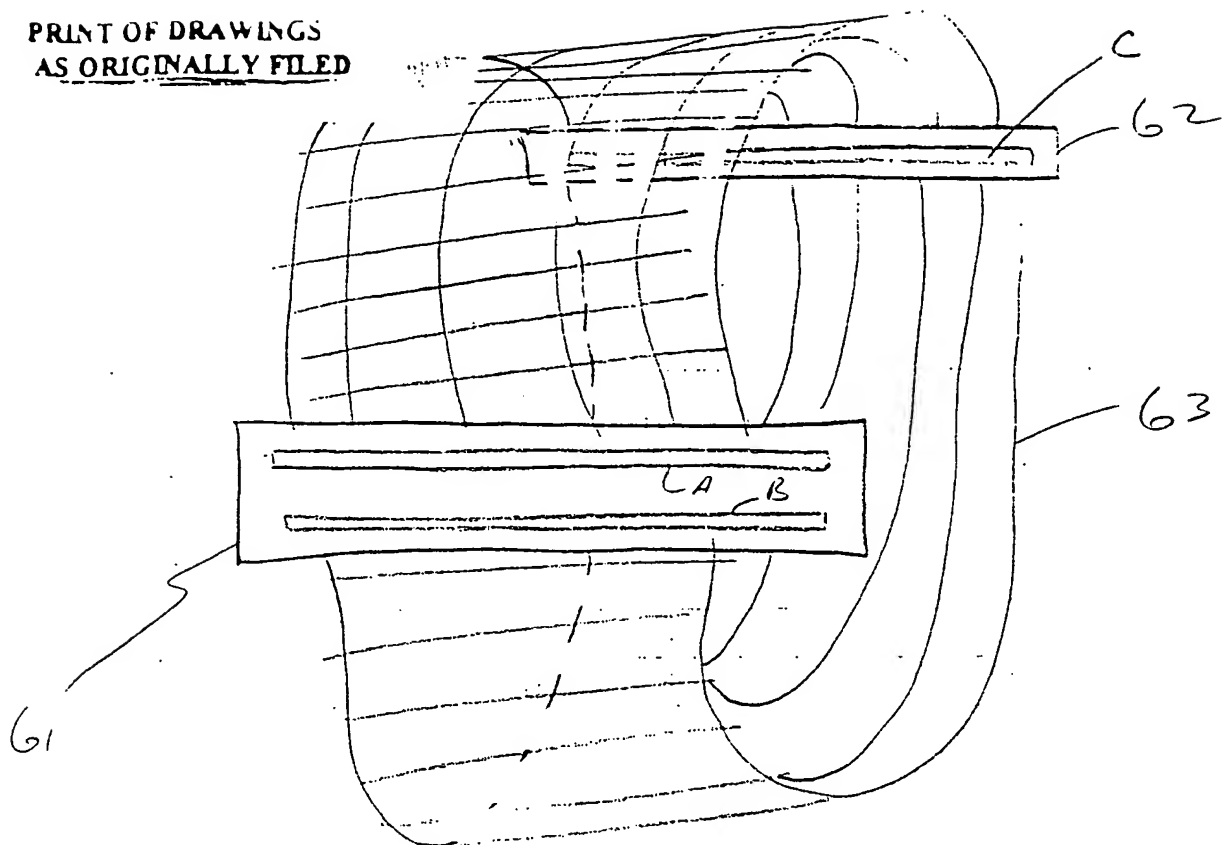


Fig. 5








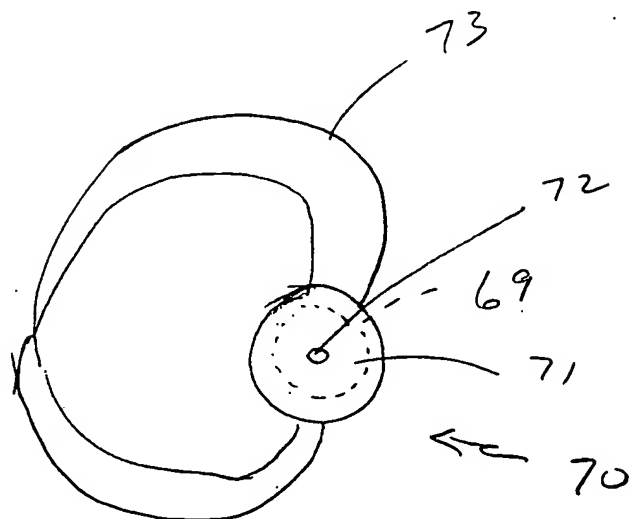


Fig. 6

00449303 112699

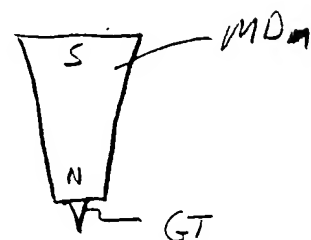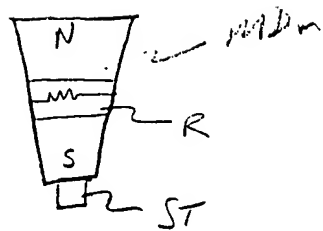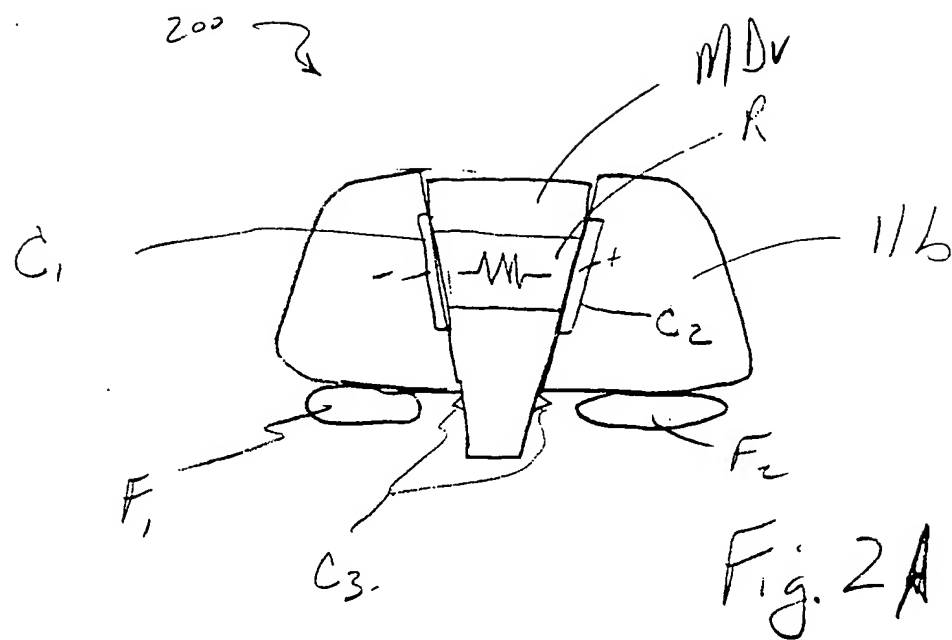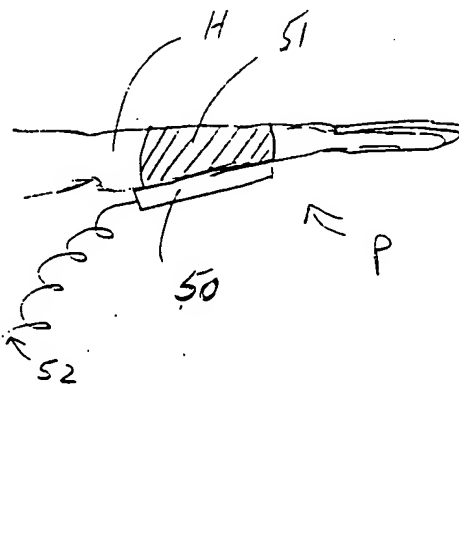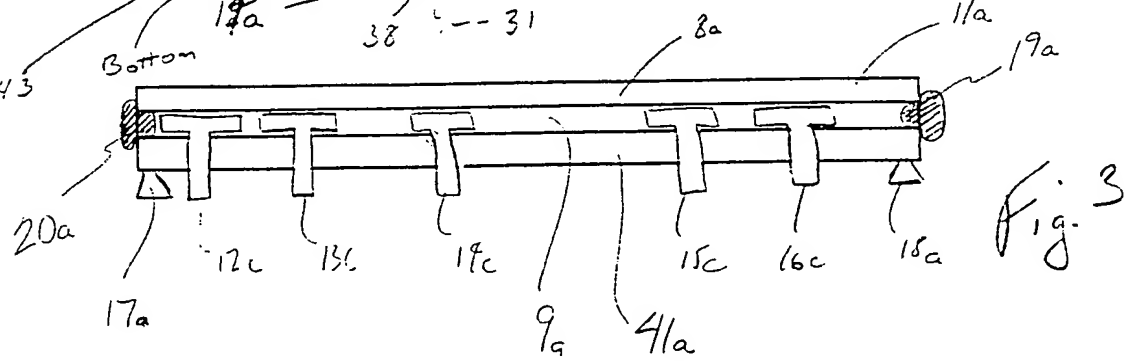

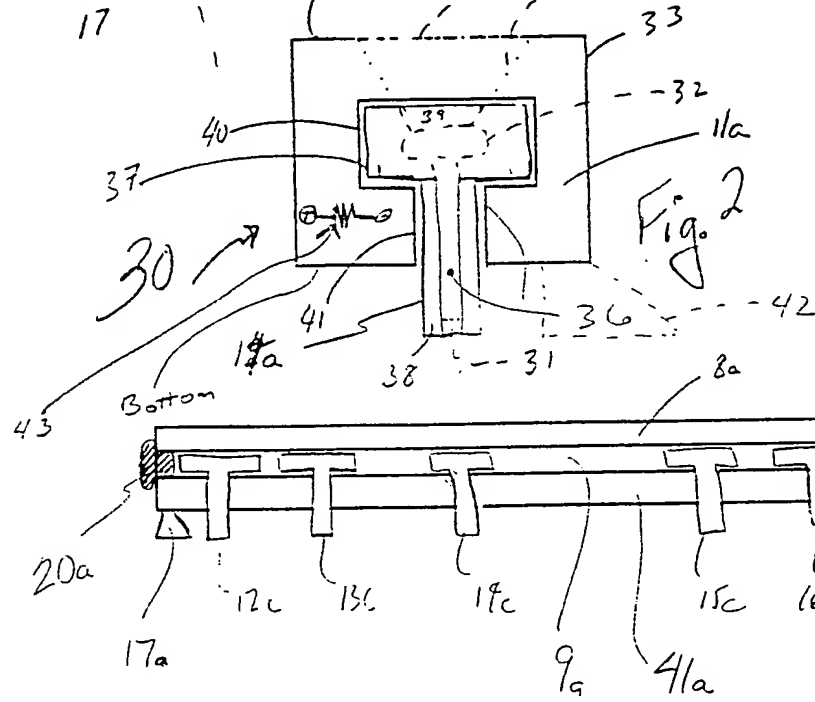

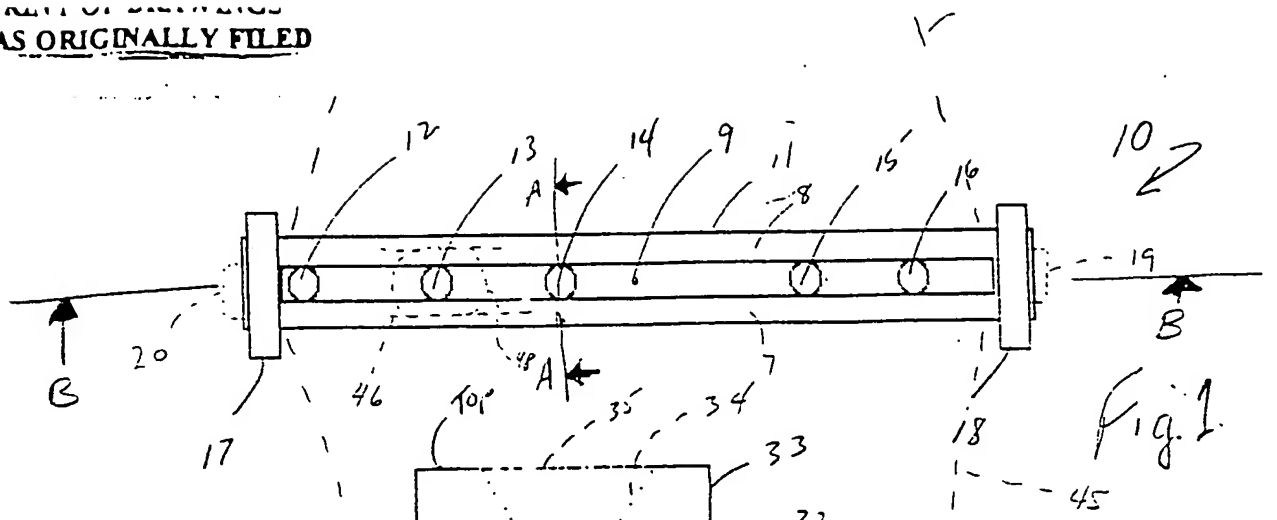

66321-1066460